


Schaltbild ISO 1000

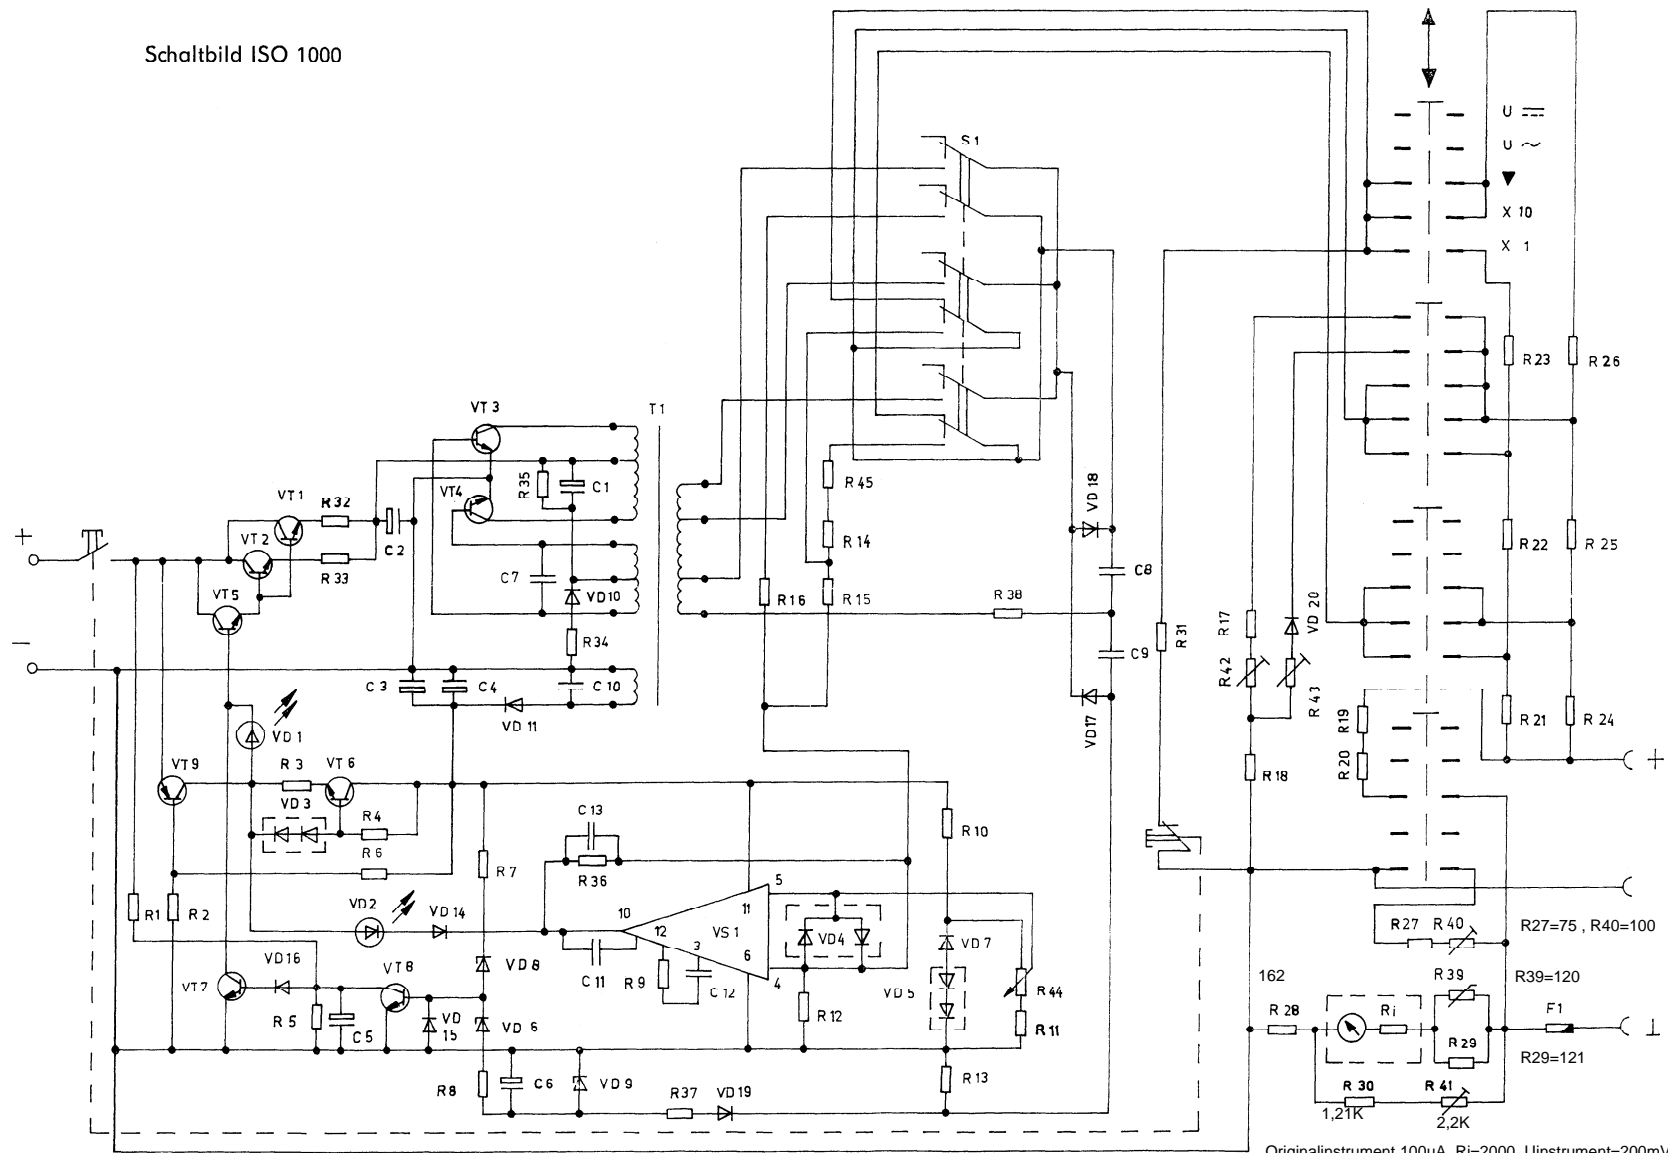

Originalinstrument 100 μ A, $R_i=2000$, $U_{\text{instrument}}=200\text{mV}$

Ersatzinstrument 30 μ A, $R_i=1730$, $U_{\text{instrument}}=52\text{mV}$